



BUNNELL™ Splints INSTRUCTIONS #13-B & 13.1-B

COMBINATION OPPENHEIMER AND COMPOSITE ELASTIC SPLINT EXTEND WRIST AND EXTEND D.I.P. JOINTS

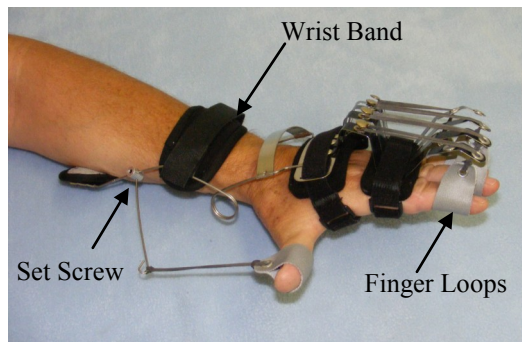

#13-B Coiled Spring Wire at Wrist

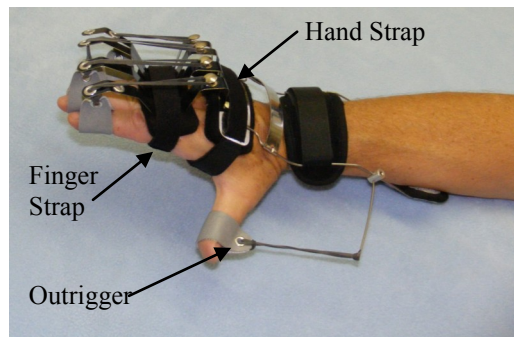

#13.1-B Straight Spring Wire at Wrist—Less extension force at wrist than #13-B

SET-UP AND ASSEMBLY

Position of the thumb outrigger determines if splint is for RIGHT or LEFT



To change position of the outrigger on the splint, loosen set screw that holds the outrigger to the lateral wire [hex key provided]. Reposition and tighten. The wire outrigger itself can be repositioned using the other set screw.

Be sure the wire end is flush with the aluminum housing when retightening. Always remove splint from patient of all adjustments.

ATTACH HAND AND FOREARM SECTIONS TOGETHER

Loosen the hand strap, reflect back, and expose openings for the forearm wire end on the forearm section.


With the hand and forearm sections in proper position, insert the wire into the opening. Be sure the wire passes completely through the opening and rests in the channel.

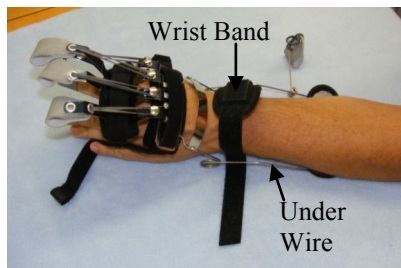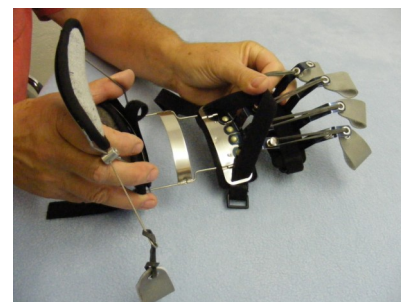

To close pass loop strap under lateral wire and back to secure with hook on top of wrist band. Wearing the wrist band/strap a little “looser” will apply less force to extend wrist.

TO DON SPLINT open wrist band and open hand and finger straps. With splint on a flat surface side hand and forearm into position. Close wrist band. Apply hand and finger straps. If necessary, apply straps with hand in a “palm up” position. Apply the finger loops. Outriggers 1 and 4 have optional positions for elastic bands. Apply thumb loop. Check and adjust position of splint. Be sure hand and finger straps are not too tight.


TO DOFF SPLINT. Avoid splint from “springing up”. Slowly and carefully remove thumb and finger loops, loosen and remove finger and hand straps, open wrist band.

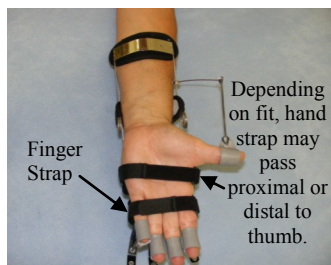

EVALUATE FIT, FUNCTION and INSTRUCT PATIENT ON USE
Splint is designed to extend wrist while allowing active wrist flexion.

TO ADJUST FORCE Remove splint and carefully bend lateral wires and or change rubber bands. Outrigger uses #31 rubber band

CLEAN with mild soap and damp towel. Remove liner, hand wash with cold water and mild detergent. Rinse thoroughly. Air dry completely before reapplication.



Avoid placing near open flame, heater, trunk of car, etc.

Immediately contact your health care professional if you are experiencing loss of sensation, swelling, skin irritations or have any questions or concerns.

CAUTION: Federal Law restricts this device to sale by or on the orders of a physician. To be dispensed by qualified healthcare professional.