

IQ Easy Alarm #711009

Instructions for Use and Care

Your new AliMed® IQ Easy Alarm includes three AAA batteries, a strap that can be used to attach the alarm to a chair, and a built-in mounting plate that can be used in combination with hook and loop to attach to a bed. This alarm features a unique sensor connector that can only be used with AliMed IQ Easy Single-Patient-Use sensor pads (bed or chair).

Battery Installation

Open the battery compartment by loosening the screw on the base of the cover. Insert batteries per guide in battery compartment.

Operating Instructions

1. Connect IQ Easy Alarm to IQ Easy Single-Patient-Use Sensor Pad by simply plugging connector into the bottom of the alarm (*Figure 1*).
2. Connection is complete when LCD located on the front of the alarm illuminates green and the alarm says, "System on." The green light signifies the alarm is on and ready to use. (*Figure 2*).
3. Load/Press sensor cable into the cable support channel on back of alarm.

Test alarm*

4. When pressure is placed on alarm, a prerecorded voice will say, "System ready" to notify caregiver that the alarm is working properly. If pressure is removed, the LCD light (*Figure 3*) will illuminate yellow and emit a 100 dB alarm sound. To reset the alarm, either reapply pressure to the pad, or press the black reset button located on the front of the alarm (*Figure 4*). A prerecorded voice will state "System reset" when reset button is pressed. If test fails, check batteries. Discontinue use if alarm fails to operate.

NOTE: To turn alarm off, simply disconnect alarm from sensor pad.

Chair and Bed Attachment

1. Use convenient strap (connected to alarm) for attaching alarm to wheelchair handle (*Figure 5*).
2. The backside of the alarm contains two slots. Slide mounting bracket into slots and cover with hook and loop to attach to bed. This mounting bracket also acts as a barrier to help eliminate tampering with sensor connection.

Manufactured for:

 **AliMed® inc.**
297 High St., Dedham, MA 02026 USA
PH 800-225-2610 • FAX 800-437-2966




Figure 1



green light

Figure 2



yellow light

Figure 3





Figure 4



nurse call connector

Figure 5

www.AliMed.com
#5974REV0811 CCO408
©2011 AliMed® inc. All rights reserved.
Made in China
GTIN: 0733657200683

IQ Easy Alarm #711009

Instructions for Use and Care

Your new AliMed® IQ Easy Alarm includes three AAA batteries, a strap that can be used to attach the alarm to a chair, and a built-in mounting plate that can be used in combination with hook and loop to attach to a bed. This alarm features a unique sensor connector that can only be used with AliMed IQ Easy Single-Patient-Use sensor pads (bed or chair).

Battery Installation

Open the battery compartment by loosening the screw on the base of the cover. Insert batteries per guide in battery compartment.

Operating Instructions

1. Connect IQ Easy Alarm to IQ Easy Single-Patient-Use Sensor Pad by simply plugging connector into the bottom of the alarm (*Figure 1*).
2. Connection is complete when LCD located on the front of the alarm illuminates green and the alarm says, "System on." The green light signifies the alarm is on and ready to use. (*Figure 2*).
3. Load/Press sensor cable into the cable support channel on back of alarm.

Test alarm*

4. When pressure is placed on alarm, a prerecorded voice will say, "System ready" to notify caregiver that the alarm is working properly. If pressure is removed, the LCD light (*Figure 3*) will illuminate yellow and emit a 100 dB alarm sound. To reset the alarm, either reapply pressure to the pad, or press the black reset button located on the front of the alarm (*Figure 4*). A prerecorded voice will state "System reset" when reset button is pressed. If test fails, check batteries. Discontinue use if alarm fails to operate.

NOTE: To turn alarm off, simply disconnect alarm from sensor pad.

Chair and Bed Attachment

1. Use convenient strap (connected to alarm) for attaching alarm to wheelchair handle (*Figure 5*).
2. The backside of the alarm contains two slots. Slide mounting bracket into slots and cover with hook and loop to attach to bed. This mounting bracket also acts as a barrier to help eliminate tampering with sensor connection.

Manufactured for:

 **AliMed® inc.**
297 High St., Dedham, MA 02026 USA
PH 800-225-2610 • FAX 800-437-2966



Figure 1



green light

Figure 2



yellow light

Figure 3




Figure 4



nurse call connector

Figure 5

www.AliMed.com
#5974REV0811 CCO408
©2011 AliMed® inc. All rights reserved.
Made in China
GTIN: 0733657200683

Specialized Features

- Voice feature—Alerts caregiver when alarm is on, armed, reset, or has a low battery
- “System on” sound is emitted when sensor pad is correctly connected to alarm
- “System reset” sound is emitted when reset button is pressed
- “System ready” sound is emitted when pressure is placed on pad
- “Low battery” sound is emitted when alarm has low battery levels; Batteries must be replaced in order to silence
- A unique Nurse Call connector slot located on side of the alarm (*Figure 5*) can be combined with the IQ Easy nurse call cable that will enable the alarm to sound in the room and at the nurse call station.
- LCD light located on the front of the alarm (*Figure 2*) will illuminate green, red and yellow
 - Green – signifies alarm is ready to use
 - Yellow – signifies when alarm is sounding or set off
 - Red – signifies low battery power

Warnings

- a) AliMed alarms alert caregivers to attend to patients or residents who have either risen or are about to rise. They do not prevent falls.
- b) Discontinue use immediately if unit is damaged, incomplete, or the back compartment cover is missing.

NOTE:

*Test alarm daily to ensure patient safety.

Care

Wipe clean using standard cleaning disinfectants. Do not immerse in fluids. Check function of alarm before each use.

Construction


ABS plastic.

To Reorder

- #71 2123 IQ Easy w/Single-Patient-Use Bed Sensor Pad
- #71 2124 IQ Easy w/Single-Patient-Use Chair Sensor Pad
- #71 2121 IQ Easy Single-Patient-Use Bed Sensor Pad
- #71 2175 IQ Easy Single-Patient-Use Bed Sensor Pad, 10/cs
- #71 2122 IQ Easy Single-Patient-Use Chair Sensor Pad
- #71 2176 IQ Easy Single-Patient-Use Chair Sensor Pad, 10/cs

IQ Duo Plus Alarm is the most versatile alarm available. It functions as either a magnetic pull-cord alarm or a sensor-pad alarm by flicking a switch. It is compatible with all of AliMed’s sensor pad, seatbelt, or alarm strap systems.

85- or 100-dB alarm setting • Single concealed reset button • Chime or alarm alert • Silent feature when used in combination with the nurse call jack alarm, can be set to silent in patient’s room • Low-battery light • Mounting holster • Nurse call jack • Rubber bumpers • For use as a pull cord or with sensor devices—sensor pads bed/chair, seatbelts, bed belt, cushions • Adjustable pull-cord • 3 AAA batteries included

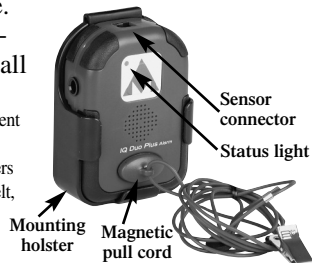

#71 1290 IQ Duo Plus Alarm

Manufactured for:

 **AliMed® inc.**
297 High St., Dedham, MA 02026 USA
PH 800-225-2610 • FAX 800-437-2966

www.AliMed.com
#5974REV0811 CCO408
©2011 AliMed® inc. All rights reserved.
Made in China
GTIN: 0733657200683

Specialized Features

- Voice feature—Alerts caregiver when alarm is on, armed, reset, or has a low battery
- “System on” sound is emitted when sensor pad is correctly connected to alarm
- “System reset” sound is emitted when reset button is pressed
- “System ready” sound is emitted when pressure is placed on pad
- “Low battery” sound is emitted when alarm has low battery levels; Batteries must be replaced in order to silence
- A unique Nurse Call connector slot located on side of the alarm (*Figure 5*) can be combined with the IQ Easy nurse call cable that will enable the alarm to sound in the room and at the nurse call station.
- LCD light located on the front of the alarm (*Figure 2*) will illuminate green, red and yellow
 - Green – signifies alarm is ready to use
 - Yellow – signifies when alarm is sounding or set off
 - Red – signifies low battery power

Warnings

- a) AliMed alarms alert caregivers to attend to patients or residents who have either risen or are about to rise. They do not prevent falls.
- b) Discontinue use immediately if unit is damaged, incomplete, or the back compartment cover is missing.

NOTE:

*Test alarm daily to ensure patient safety.

Care

Wipe clean using standard cleaning disinfectants. Do not immerse in fluids. Check function of alarm before each use.

Construction


ABS plastic.

To Reorder

- #71 2123 IQ Easy w/Single-Patient-Use Bed Sensor Pad
- #71 2124 IQ Easy w/Single-Patient-Use Chair Sensor Pad
- #71 2121 IQ Easy Single-Patient-Use Bed Sensor Pad
- #71 2175 IQ Easy Single-Patient-Use Bed Sensor Pad, 10/cs
- #71 2122 IQ Easy Single-Patient-Use Chair Sensor Pad
- #71 2176 IQ Easy Single-Patient-Use Chair Sensor Pad, 10/cs

IQ Duo Plus Alarm is the most versatile alarm available. It functions as either a magnetic pull-cord alarm or a sensor-pad alarm by flicking a switch. It is compatible with all of AliMed’s sensor pad, seatbelt, or alarm strap systems.

85- or 100-dB alarm setting • Single concealed reset button • Chime or alarm alert • Silent feature when used in combination with the nurse call jack alarm, can be set to silent in patient’s room • Low-battery light • Mounting holster • Nurse call jack • Rubber bumpers • For use as a pull cord or with sensor devices—sensor pads bed/chair, seatbelts, bed belt, cushions • Adjustable pull-cord • 3 AAA batteries included

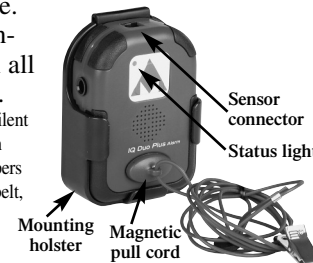

#71 1290 IQ Duo Plus Alarm

Manufactured for:

 **AliMed® inc.**
297 High St., Dedham, MA 02026 USA
PH 800-225-2610 • FAX 800-437-2966

www.AliMed.com
#5974REV0811 CCO408
©2011 AliMed® inc. All rights reserved.
Made in China
GTIN: 0733657200683