


# Cubital Comfort Brace


## Warnings and Instructions: Review carefully, proper application is required

**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Over-tighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.


**Care:** Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

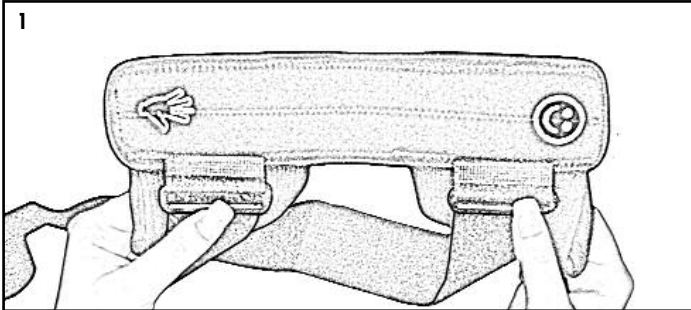


1. For orientation, check the brace for the head and hand symbols.

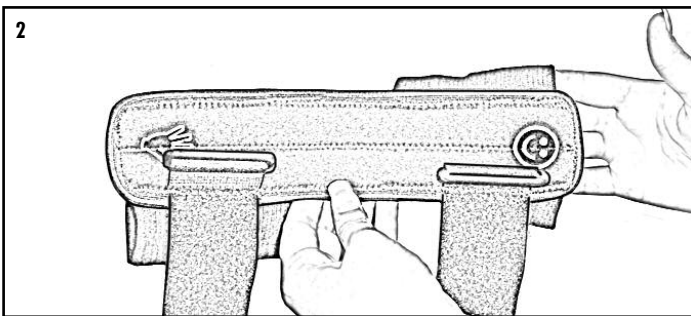


2. The brace should be applied on the arm with the head icon on the upper arm (towards the head) and the hand icon on the lower arm (towards the hand) by sliding the brace on the arm through the stockinette sleeves.

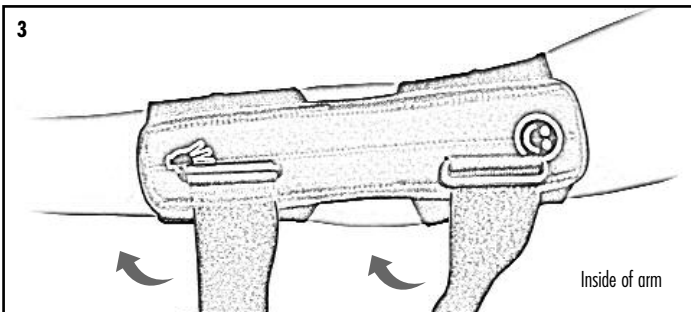



3. The brace should be positioned with the bend in the stays centered over the elbow crease.

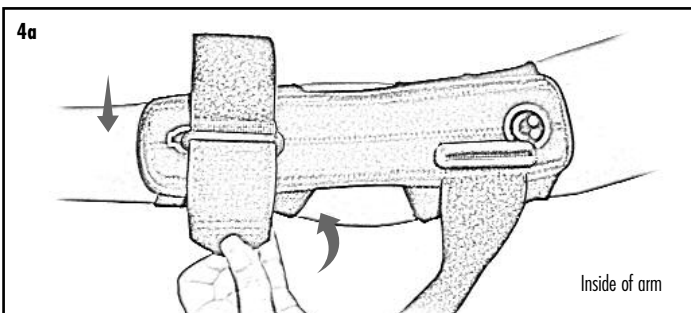

4a. The brace is then secured with the hook and loop straps.

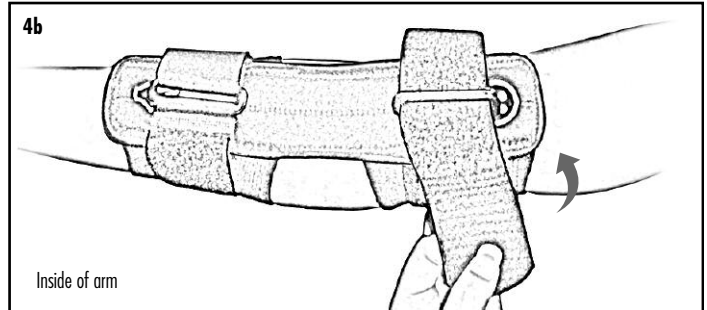

4b. The brace should be tight enough to maintain the brace in position, but not too tight as to interfere with circulation.

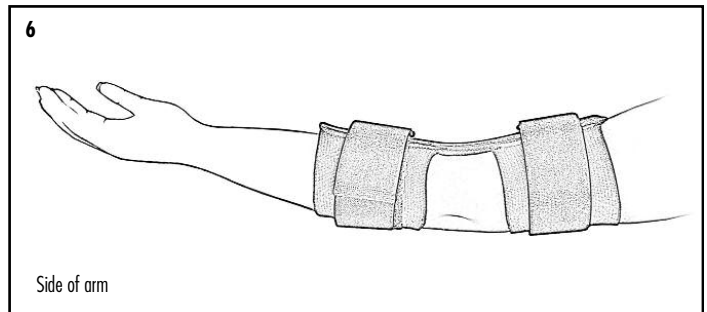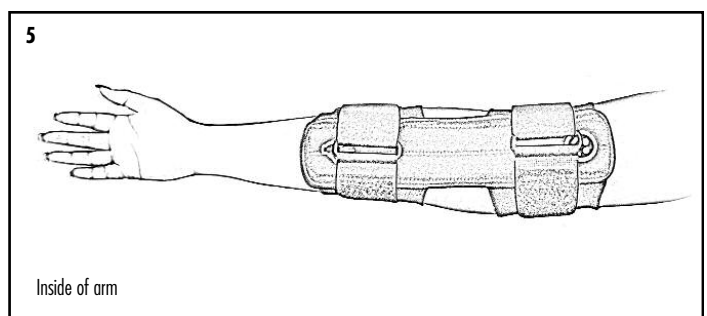

The Cubital Comfort Brace was designed for the treatment of Cubital Tunnel Syndrome, compression of the ulnar nerve at the elbow. The brace keeps the elbow in a relatively straight position. This keeps the ulnar nerve in a relaxed position, where it is neither in compression nor tension. The brace may be used for other conditions as well (when maintaining a straight elbow position is desired). It is typically worn at bedtime, but can be worn at anytime.

## The Cubital Comfort Brace comes in 2 sizes.

U.S. Patent No. 7074202, D523961

**HELLY & WEBER**

© 2007 Weber Orthopedic Inc.  
DBA Hely & Weber All rights reserved.  
1185 East Main St., Santa Paula, California 93060  
California: 800-221-5465, National: 800-654-3241  
International: 805-525-4244, fax: 805-933-2348  
U.S. fax: 800-559-5975, www.hely-weber.com

**CE**

EC REP

MDSS GmbH  
Schiffgraben 41  
30175 Hannover, Germany

Rev A 11/08