


Weblly Ankle Orthosis


Warnings and Instructions: Review carefully, proper application is required

Warning: This device will not prevent or eliminate risk of injury. Do Not Over-tighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

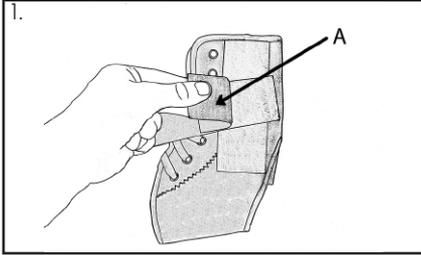


1. Separate the top hook strap-locks (A) from the straps on both sides of the brace.

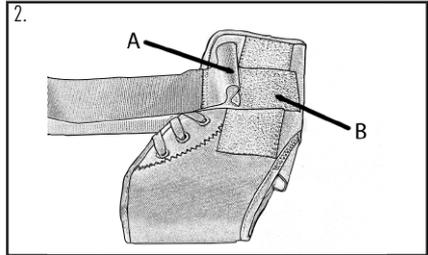


2. Temporarily attach the top hook strap-locks (A) to the straps so the loop material underneath (B) is exposed.

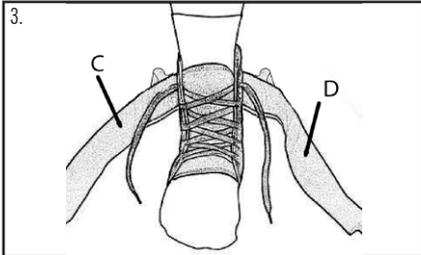


3. The Weblly Ankle Orthosis is designed to be worn over an athletic sock. Position your heel into the hole at the rear and bottom of the brace. Tighten the laces snugly and tie.

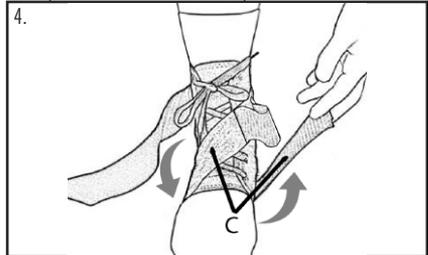


4. Bring the inside strap (C) forward, across the top of the foot. Wrap it under the foot, continuing under the heel, and pull the strap upward securing the hook fastener onto the loop material on the inside of the ankle.

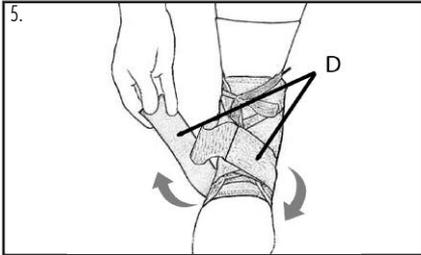

5. Bring the outside strap (D) forward, across the top of the foot. Wrap it under the heel, and pull the strap upward, securing the hook fastener onto the loop material on the outside of the ankle.

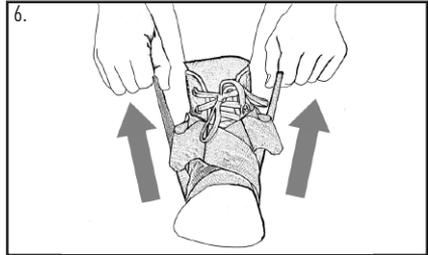

6. Stand, putting full weight on your ankle, pull up on both straps simultaneously to gain proper alignment and tightness. Attach the hook fasteners of the straps onto loop material.

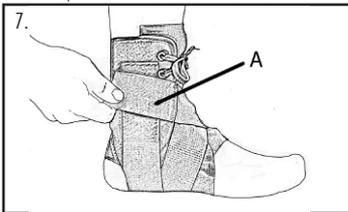

7. Attach the top hook strap-locks (A) over the straps. If strap lengths are too long, conveniently trim.

HELLY & WEBER

© 2009 Weber Orthopedic Inc.
DBA Helly & Weber All rights reserved.

1185 East Main St., Santa Paula, California 93060
California: 800-221-5465, National: 800-654-3241
International: 805-525-4244, fax: 805-933-2348
U.S. fax: 800-559-5975, www.helly-weber.com

U.S. Patent No. 6117098



EC REP

MDS5 GmbH
Schiffgraben 41
30175 Hannover, Germany

Rev A 11/08