




Wrist Support

Single Patient Use Only • Rx Only

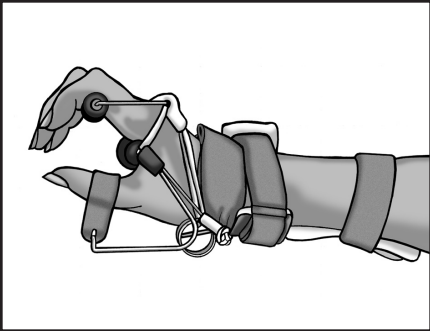

IMPORTANT INFORMATION

The following information should be read prior to use of this device.

INTENDED USE

The Wrist Support uses wire coils at the wrist joint axis to assist the wrist and digits into extension. The thumb outrigger assists the thumb into abduction/extension. This splint is recommended in injuries involving the radial nerve.

Splint size is determined by the width of the hand at the metacarpophalangeal joints.

Small female

B 2 1/4" – 2 3/4" 5.71 – 6.98 cm

Average female, small male


C 2 7/8" – 3 1/4" 7.28 – 8.26 cm

Average to large male

D 3 3/8" – 3 3/4" 8.57 – 9.53 cm


DIRECTIONS FOR USE

1. To fit the splint, loosen all strapping from the radial side. Slide hand into splint so the




contoured palm support rests in the palmar arch and the distal bar rests along the volar surface of the proximal phalanx of the fingers.

2. When strapping the elastic wrist strap, note that the strap remains fastened around the ulnar coil. Cross the strap over the wrist. Wrap the strap around the wire extending from the radial coil. Adhere the loop material to the hook material. Once fastened, the strap will rest along the dorsum of the wrist.




3. On the wrist, attach the folded end of the Duraval® to the radial side of the splint.




Secure the splint at the wrist by pulling the strap through the ulnar slit and adhering it to the adjacent hook material. Securing the splint will position the ulnar support close to the wrist.

4. To strap the forearm, wrap the Duraval® strap around forearm so the hook material



Wrist Support

Single Patient Use Only • Rx Only

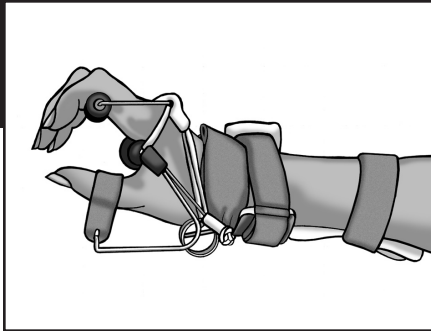

IMPORTANT INFORMATION

The following information should be read prior to use of this device.

INTENDED USE

The Wrist Support uses wire coils at the wrist joint axis to assist the wrist and digits into extension. The thumb outrigger assists the thumb into abduction/extension. This splint is recommended in injuries involving the radial nerve.

Splint size is determined by the width of the hand at the metacarpophalangeal joints.

Small female

B 2 1/4" – 2 3/4" 5.71 – 6.98 cm

Average female, small male


C 2 7/8" – 3 1/4" 7.28 – 8.26 cm

Average to large male

D 3 3/8" – 3 3/4" 8.57 – 9.53 cm


DIRECTIONS FOR USE

1. To fit the splint, loosen all strapping from the radial side. Slide hand into splint so the




contoured palm support rests in the palmar arch and the distal bar rests along the volar surface of the proximal phalanx of the fingers.

2. When strapping the elastic wrist strap, note that the strap remains fastened around the ulnar coil. Cross the strap over the wrist. Wrap the strap around the wire extending from the radial coil. Adhere the loop material to the hook material. Once fastened, the strap will rest along the dorsum of the wrist.




3. On the wrist, attach the folded end of the Duraval® to the radial side of the splint.



Secure the splint at the wrist by pulling the strap through the ulnar slit and adhering it to the adjacent hook material. Securing the splint will position the ulnar support close to the wrist.


4. To strap the forearm, wrap the Duraval® strap around forearm so the hook material






on the folded end of Duraval® makes contact with strap along the volar surface of the splint. Trim excess strapping.

5. To increase the wrist extension, bend the lateral wires into extension force. The bend should be equal



in the radial and ulnar wire. Slide the plastic tubes up along the elastic attached to the finger outrigger. This brings the fingers into extension. Tie the elastic and cut.

6. With the hand positioned in the splint, slide the thumb cuff on the thumb so it rests at the proximal



phalanx. The wire attached to the thumb cuff can be adjusted for desired thumb extension/abduction.

PRECAUTIONS

These products are to be fitted initially by a healthcare professional who is familiar with the purpose for which they are used.

The healthcare professional is responsible for providing wearing instructions and precautions to other healthcare professionals, care providers involved in the patient's care, and the patient. If unusual swelling, skin discoloration or discomfort occurs, use should be discontinued and a healthcare professional consulted.

CARE INSTRUCTIONS

Straps may be removed and laundered. Splint surface may be cleansed with a mild, non-abrasive detergent and water. Air dry prior to wearing.




Manufacturer
DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Part #1-708
©2009 DeRoyal. All Rights Reserved.
Revised 1/09




on the folded end of Duraval® makes contact with strap along the volar surface of the splint. Trim excess strapping.

5. To increase the wrist extension, bend the lateral wires into extension force. The bend should be equal



in the radial and ulnar wire. Slide the plastic tubes up along the elastic attached to the finger outrigger. This brings the fingers into extension. Tie the elastic and cut.

6. With the hand positioned in the splint, slide the thumb cuff on the thumb so it rests at the proximal



phalanx. The wire attached to the thumb cuff can be adjusted for desired thumb extension/abduction.

PRECAUTIONS

These products are to be fitted initially by a healthcare professional who is familiar with the purpose for which they are used.

The healthcare professional is responsible for providing wearing instructions and precautions to other healthcare professionals, care providers involved in the patient's care, and the patient. If unusual swelling, skin discoloration or discomfort occurs, use should be discontinued and a healthcare professional consulted.

CARE INSTRUCTIONS

Straps may be removed and laundered. Splint surface may be cleansed with a mild, non-abrasive detergent and water. Air dry prior to wearing.



Manufacturer
DeRoyal
200 DeBusk Lane
Powell, TN 37849 U.S.A.
888.938.7828
865.938.7828

Part #1-708
©2009 DeRoyal. All Rights Reserved.
Revised 1/09